
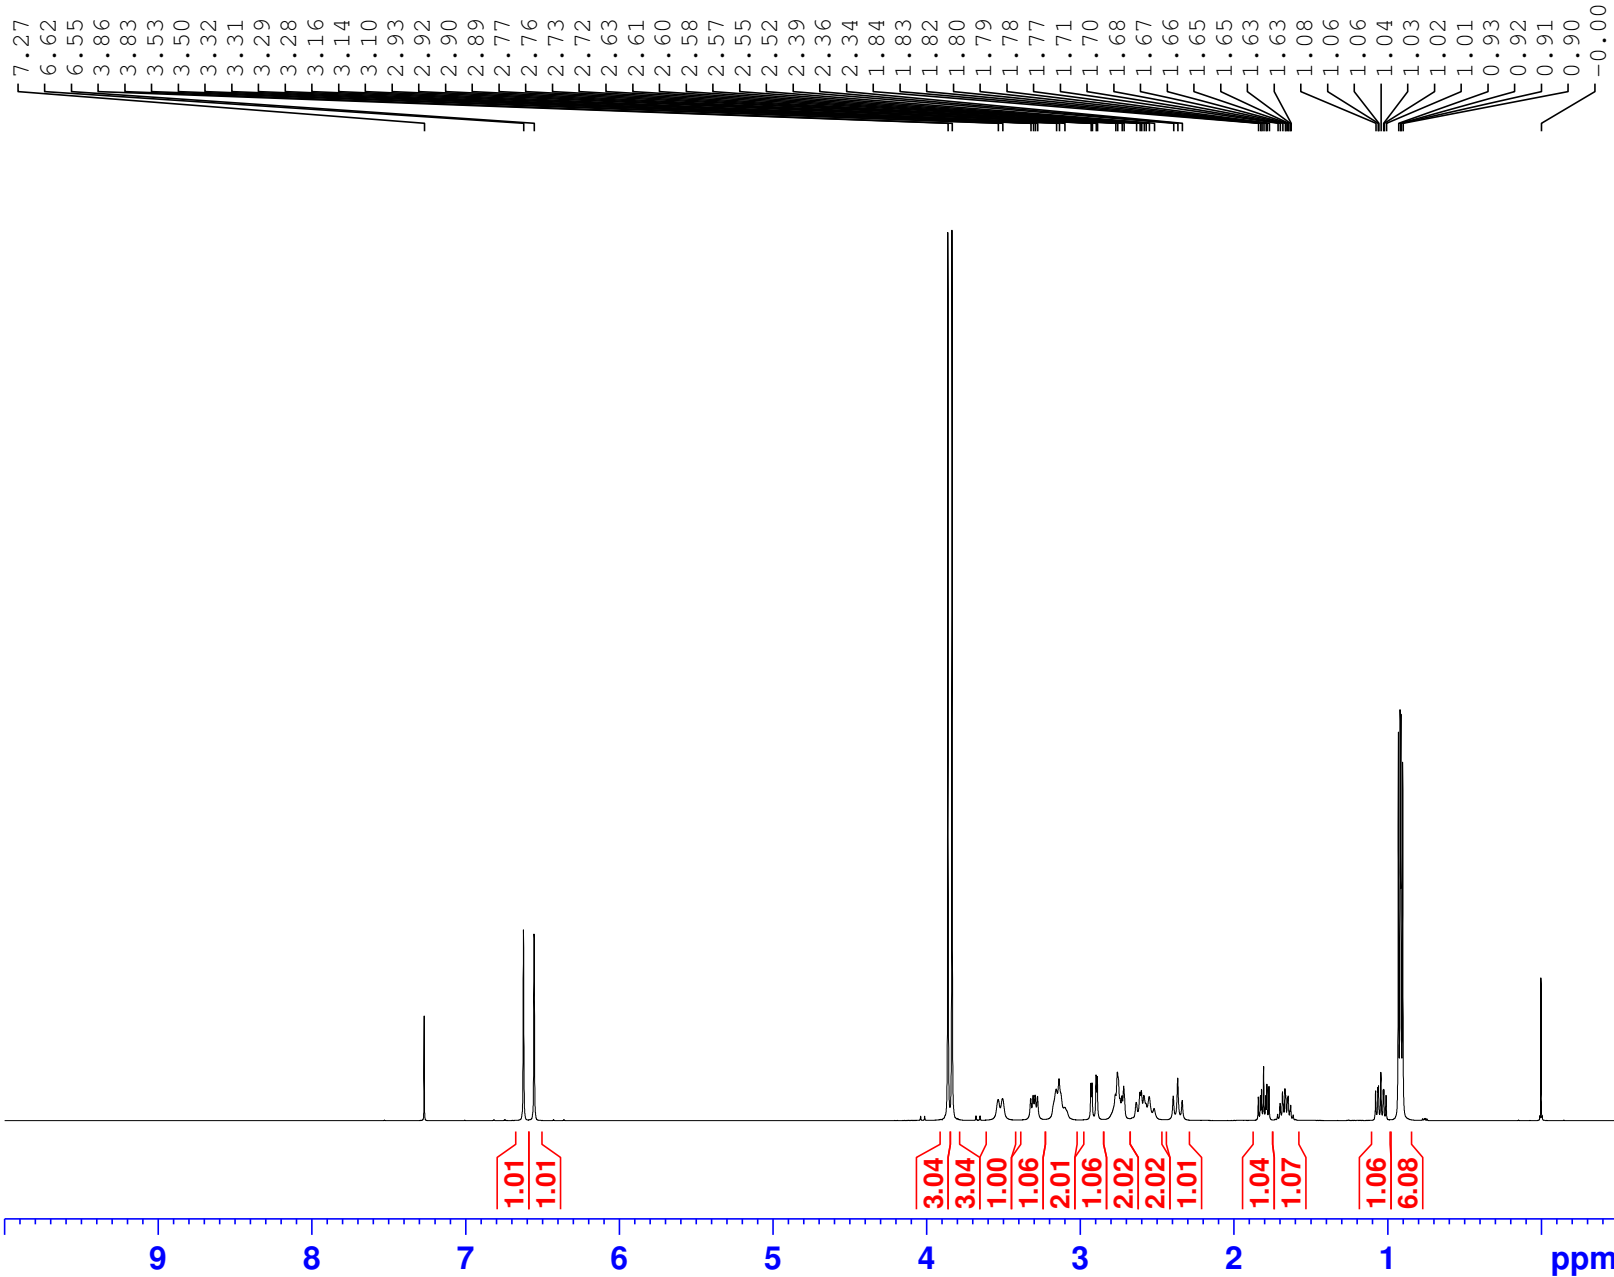


230629 CDC13

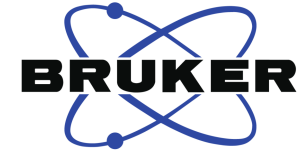

Current Data Parameters  
 NAME 230629  
 EXPNO 1  
 PROCNO 1

F2 - Acquisition Parameters  
 Date\_ 20230705  
 Time 16.03 h  
 INSTRUM spect  
 PROBHD Z116098\_0470 (  
 PULPROG zg30  
 TD 65536  
 SOLVENT CDC13  
 NS 16  
 DS 2  
 SWH 8012.820 Hz  
 FIDRES 0.244532 Hz  
 AQ 4.0894465 sec  
 RG 72.07  
 DW 62.400 usec  
 DE 6.50 usec  
 TE 294.9 K  
 D1 1.00000000 sec  
 TD0 1  
 SFO1 400.1324708 MHz  
 NUC1 1H  
 P1 12.00 usec  
 PLW1 11.86200047 W

F2 - Processing parameters  
 SI 65536  
 SF 400.1300148 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00